



Dosing Guidelines

SenTiva™



Phase 1: Output Current

Increase Output Current to therapeutic effect as tolerated by the patient

NORMAL MODE: 0.25 mA steps to therapeutic effect^{1,2}

AUTOSTIM MODE*: Normal Mode + 0.125 mA
AutoStim should be comfortable for patients

MAGNET MODE: Normal Mode + 0.25 mA
Magnet Mode should be > than AutoStim Mode

Standard Protocol

		Visit	1	2	3	4	5	6	7
NORMAL	Output Current	mA	0.25	0.5	0.75	1.0	1.25	1.5	1.75
	Signal Frequency	Hz	20	20	20	20	20	20	20
	Pulse Width	μsec	250	250	250	250	250	250	250
	Signal ON Time	seconds	30	30	30	30	30	30	30
	Signal OFF Time	minutes	5	5	5	5	5	5	5
AUTOSTIM	Output Current	mA	0.375	0.625	0.875	1.125	1.375	1.625	1.875
	Pulse Width	μsec	250	250	250	250	250	250	250
	ON Time	seconds	60	60	60	60	60	60	60
MAGNET	Output Current	mA	0.5	0.75	1.0	1.25	1.5	1.75	2.0
	Pulse Width	μsec	500	500	500	500	500	500	500
	ON Time	seconds	60	60	60	60	60	60	60


- ▶ Suggested programming settings ≥ 2 weeks post-op
- ▶ More frequent visits (1 - 2 weeks) are suggested in Phase 1
- ▶ Multiple 0.25 mA increases may be made in a single visit to reach therapeutic range sooner; ensure

Dosing Notes

- ▶ Continue to optimize dose to therapeutic effect or tolerability
- ▶ Give patient time to adapt to parameter changes before making additional adjustments

Phase 2: Duty Cycle

- ▶ Increase duty cycle over time and assess clinical outcome
- ▶ Adjustments to duty cycle should be less frequent (3 - 6 months)

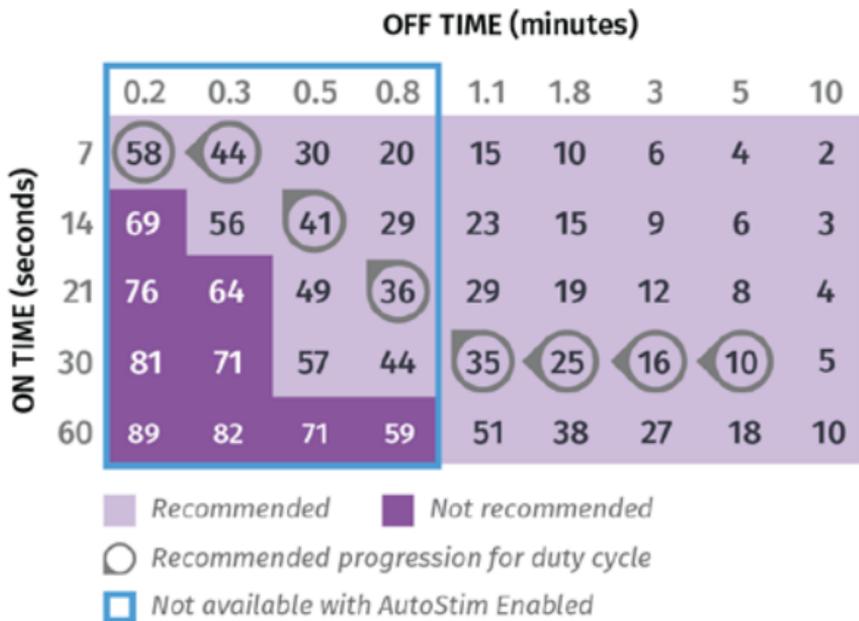

LivaNova recommends that stimulation with Normal Mode ON time > OFF time be avoided. Duty Cycle = (ON Time + 4 seconds) / (ON time + OFF Time), for which ON and OFF Time are measured in seconds.

Additional Settings for SenTiva

Tachycardia Detection	ON/OFF
Heartbeat Detection* Range (1 - 5)	Set at Sensitivity 3 and verify heartbeat detection Adjust setting if necessary, until accurate detection is reached
Threshold for AutoStim* (% heart rate increase) Range (20 - 70%)	Set at or below the patient's typical heart rate increase during a seizure If not available, start with 20% and adjust based on clinical benefit or tolerability
Prone Position*	Configure generator to log the occurrence of prone position when they occur within 7.5 minutes of an AutoStim or Magnet Mode activation
Low Heart Rate* Range (30-60 BPM)	Configure generator to log low heart rate episodes when they occur within 7.5 minutes of an AutoStim or Magnet Mode activation

*Tachycardia detection must be enabled

Strategies to Manage Side Effects

- ▶ Evaluate tolerability after each adjustment
- ▶ Side effects typically decrease over time^{3,4}

RECOMMENDED ORDER	
1. Pulse Width	If 500 → 250 μsec^{\dagger}
2. Signal Frequency	If 30 → 25 or 20 Hz^{\S}
3. Output Current	↓ 0.125 mA ↓ 0.25 mA
FOR AUTOSTIM-RELATED SIDE EFFECTS*	
1. Verify Heartbeat Detection	Adjust Heartbeat Detection sensitivity, if necessary
2. AutoStim Parameters	↓ Pulse Width ↓ Output Current (0.125 mA) ↓ ON Time
3. Threshold for AutoStim	↑ 10%

Guided Programming

Establishes a safe and easy pathway towards achieving targeted therapy levels through one touch programming. Follow an FDA-approved Standard Protocol or create a protocol.

1. **Interrogate** the generator
2. Go to **Parameters** screen
3. Switch to **Guided Mode**
4. Select **Standard Protocol** or **Custom Protocol** and Tap **Next**
See Physician's Manual for information on custom protocols
5. Review changes and select **Apply Changes**

To increase parameters:

- A. Select **Increase step**
- B. Review step increase and **Apply Changes**


6. or

To decrease parameters:

- A. Select **Decrease step**
- B. Review step decrease and **Apply Changes**

7. **Interrogate**

8. Press **End Session**

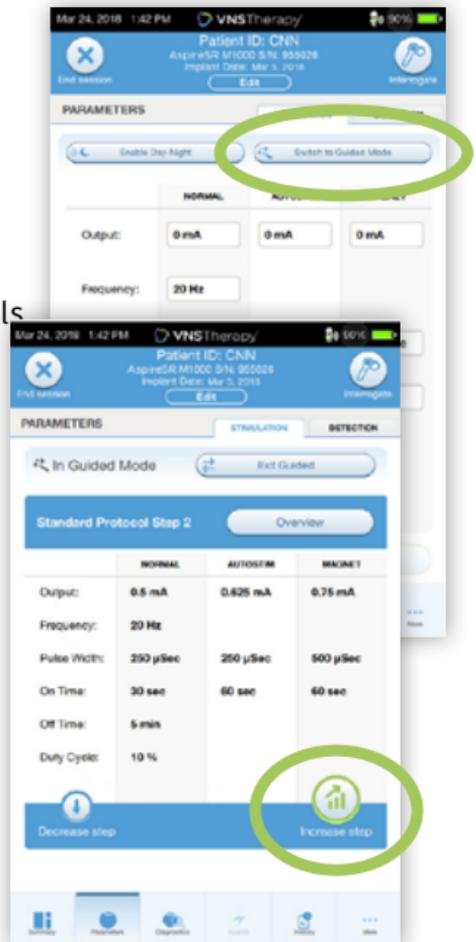

[†] Lower than 250 μsec not recommended

[§] Lower than 20Hz not recommended

Scheduled Programming


Optional feature allowing the programming of a titration schedule in one office visit. The titration changes will be applied at the defined intervals while the patient lives their life. Follow an FDA-approved Standard Protocol or create a custom protocol.

To use this feature, the generator must be in Guided Mode:

See Guided Programming steps

To turn on Scheduled Programming follow these steps:

1. In Guided Mode, select the **SCHEDULED-APPLY** button
2. On the Scheduled-Apply Screen, select **ENABLE NOW**
3. Select the time interval between step increases, then select **GENERATE SCHEDULE***
4. Once a schedule has been generated, edit the date(s) and time(s) for programming changes if necessary.
Select **APPLY CHANGES** to program changes

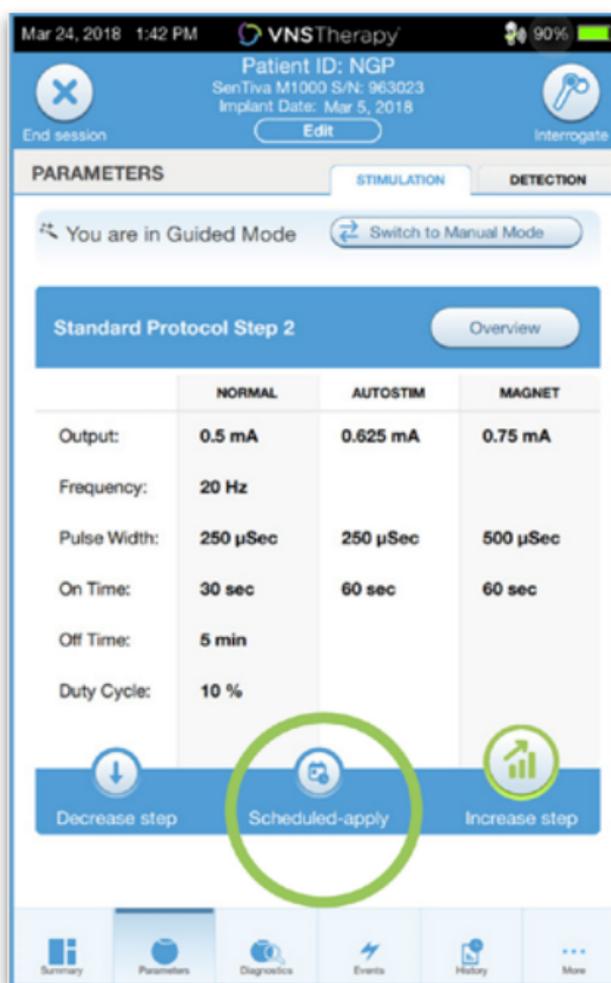

NOTE: At the end of each office visit, the generator must be interrogated by selecting **INTERROGATE** followed by **END SESSION** to ensure creation and accuracy of the Session Reports

* Limited to 0.25 mA increases every 14+ days or 0.125 mA every 7 days

See VNS Therapy Physician's Manual for complete information on programming and diagnostics.

Analysis / Programming CPT-4 Codes (All Settings)

CPT Code	Description
FULL SYSTEM IMPLANT (ELECTRODE AND GENERATOR)	
95970	Electronic analysis of implanted neurostimulator pulse generator/transmitter (eg, contact group[s], interleaving, amplitude, pulse width, frequency [Hz], on/off cycling, burst, magnet mode, dose lockout, patient selectable parameters, responsive neurostimulation, detection algorithms, closed loop parameters, and passive parameters) by physician or other qualified health care professional; with brain, cranial nerve, spinal cord, peripheral nerve, or sacral nerve, neurostimulator pulse generator/transmitter, without programming
95976	Electronic analysis with simple cranial nerve neurostimulator pulse generator/transmitter programming by physician or other qualified health care professional (one to three parameters)
95977	Electronic analysis with complex cranial nerve neurostimulator pulse generator/transmitter programming by physician or other qualified health care professional (more than three parameters)

LivaNova has compiled this coding information for your convenience. It is the provider's responsibility to file claims with appropriate ICD-10, CPT-4, HCPCS, revenue, and/or APC codes along with charges for the services provided. Please contact your local payer if you have questions regarding appropriate coding guidelines.

Current Procedural Terminology (CPT) is copyright 2019 American Medical Association. All Rights Reserved. No fee schedules, basic units, relative values, or related listings are included in CPT. The AMA assumes no liability for the data contained herein. Applicable FARS/DFARS restrictions apply to government use. CPT® is a trademark of the American Medical Association.

Additional Information

Please see important safety information or visit www.VNSTherapy.com.

The VNS Therapy System is indicated for use as an adjunctive therapy in reducing the frequency of seizures in patients 4 years of age and older with partial onset seizures that are refractory to antiepileptic medications.

Incidence of adverse events following stimulation (>5%) were voice alteration, increased coughing, pharyngitis, paresthesia, dyspnea, dyspepsia, and nausea.

This information is not intended to serve as a substitute for a complete and thorough understanding of the material presented in the Physician's Manuals for the VNS Therapy system and its component parts and does not represent full disclosure of all pertinent information concerning the use of this product, potential safety complications, or efficacy outcomes.

REFERENCES: 1. Helmers SL, et al. Application of a computational model of vagus nerve stimulation. *Acta Neurol Scand.* 2012 Nov;126(5):336-43. 2. Heck C, Helmers SL, DeGiorgio CM. Vagus nerve stimulation therapy, epilepsy, and device parameters: scientific basis and recommendations for use. *Neurology.* 2002 Sep 24;59(6 Suppl 4):S31-7. 3. Morris GL III, Mueller WM. The Vagus Nerve Stimulation Study Group E01-E05. Long-term treatment with vagus nerve stimulation in patients with refractory epilepsy. *Neurology.* 1999;53(7):1731-1735. 4. Ben-Menachem E. Vagus nerve stimulation, side effects, and long-term safety. *J Clin Neurophysiol.* 2001;18(5):415-418.

LivaNova USA, Inc.
100 Cyberonics Boulevard
Houston, Texas 77058
Tel: +1.800.332.1375
Fax: +1.281.218.9332

LivaNova Belgium NV
Ikaroslaan 83
1930 Zaventem, Belgium
Tel: +32.2.720.95.93
Fax: +32.2.720.60.53

VNS Therapy® Reimbursement
Hotline: 1.888.867.7846
reimbursement.nm@livanova.com

©2021 LivaNova USA, Inc, a wholly-owned subsidiary of LivaNova PLC. All rights reserved. LivaNova®, SenTiva®, AspireSR® and VNS Therapy® are registered trademarks of LivaNova USA, Inc.

Brief Summary¹ of Safety Information for the VNS Therapy[®] System [Epilepsy Indication] (February 2021)

1. INTENDED USE / INDICATIONS

Epilepsy (US)—The VNS Therapy System is indicated for use as an adjunctive therapy in reducing the frequency of seizures in patients 4 years of age and older with partial onset seizures that are refractory to antiepileptic medications.

2. CONTRAINDICATIONS

Vagotomy—The VNS Therapy System cannot be used in patients after a bilateral or left cervical vagotomy.

Diathermy—Do not use short-wave diathermy, microwave diathermy, or therapeutic ultrasound diathermy on patients implanted with a VNS Therapy System. Diagnostic ultrasound is not included in this contraindication.

3. WARNINGS — GENERAL

Physicians should inform patients about all potential risks and adverse events discussed in the physician's manuals. This document is not intended to serve as a substitute for the complete physician's manuals. The safety and efficacy of the VNS Therapy System have not been established for uses outside the "Intended Use/Indications" section of the physician's manuals. The safety and effectiveness of the VNS Therapy System in patients with predisposed dysfunction of cardiac conduction systems (re-entry pathway) have not been established. Post-implant electrocardiograms and Holter monitoring are recommended if clinically indicated. Postoperative bradycardia can occur among patients with certain underlying cardiac arrhythmias. It is important to follow recommended implantation procedures and intraoperative product testing described in the Implantation Procedure chapter of the physician's manuals. During the intraoperative System Diagnostics (Lead Test), infrequent incidents of bradycardia and/or asystole have occurred. If asystole, severe bradycardia (heart rate < 40 bpm), or a clinically significant change in heart rate is encountered during a System Diagnostics (Lead Test) or during initiation of stimulation, physicians should be prepared to follow guidelines consistent with Advanced Cardiac Life Support (ACLS). Difficulty swallowing (dysphagia) may occur with active stimulation, and aspiration may result from the increased swallowing difficulties. Patients with pre-existing swallowing difficulties and those with a history of drooling or hypersalivation are at greater risk for aspiration. Use of the magnet to temporarily stop stimulation while eating may mitigate the risk of aspiration. Dyspnea (shortness of breath) may occur with active VNS Therapy. Any patient with underlying pulmonary disease or insufficiency such as chronic obstructive pulmonary disease or asthma may be at increased risk for dyspnea. Patients with obstructive sleep apnea (OSA) may have an increase in apneic events during stimulation. Lowering stimulus frequency or prolonging "OFF" time may prevent exacerbation of OSA. Vagus nerve stimulation may also cause new onset sleep apnea in patients who have not previously been diagnosed with this disorder. Device malfunction could cause painful stimulation or direct current stimulation. Either event could cause nerve damage. Patients should be instructed to use the magnet to stop stimulation if they suspect a malfunction, and then to contact their physician immediately for further evaluation. Patients with the VNS Therapy System, or any part of the VNS Therapy System, implanted should have MRI procedures performed only as described in the MRI with the VNS Therapy System instructions for use. In some cases, surgery will be required to remove the VNS Therapy System if a scan using a transmit RF body coil is needed. Excessive stimulation at an excess duty cycle (that is, one that occurs when "ON" time is greater than "OFF" time) and high frequency stimulation (i.e., stimulation at ≥ 50 Hz) has resulted in degenerative nerve damage in laboratory animals. Patients who manipulate the generator and lead through the skin (Twiddler's Syndrome) may damage or disconnect the lead from the generator and/or possibly cause damage to the vagus nerve. The Wand, Programmer, and patient magnet are MR unsafe devices. These devices are projectile hazards and must not be brought into the MR scanner room.

Generators with AutoStim only—The AutoStim Mode feature should not be used in patients with clinically meaningful arrhythmias currently being managed by devices or treatments that interfere with normal intrinsic heart rate responses (e.g., pacemaker dependency, implantable defibrillator, beta adrenergic blocker medications). Patients also should not have a history of chronotropic incompetence [commonly seen in patients with sustained bradycardia (heart rate < 50 bpm)].

Generators with AutoStim only—For anticipated use of the AutoStim feature, it is important to follow the recommended pre-surgical surface assessment described in the Implantation Procedure to determine a location for the generator to reside in which it can accurately detect heart beats.

4. WARNINGS — EPILEPSY

The VNS Therapy System should only be prescribed and monitored by physicians who have specific training and expertise in the management of seizures and the use of this device. It should only be implanted by physicians who are trained in surgery of the carotid sheath and have received specific training in the implantation of this device. The VNS Therapy System is not curative. Physicians should warn patients that the VNS Therapy System is not a cure for epilepsy and that since seizures may occur unexpectedly, patients should consult with a physician before engaging in unsupervised activities, such as driving, swimming, and bathing, and in strenuous

sports that could harm them or others. Sudden unexpected death in epilepsy (SUDEP): Through August 1996, 10 sudden and unexpected deaths (definite, probable, and possible) were recorded among the 1,000 patients implanted and treated with the VNS Therapy device. During this period, these patients had accumulated 2,017 patient-years of exposure. Some of these deaths could represent seizure-related deaths in which the seizure was not observed, at night, for example. This number represents an incidence of 5.0 definite, probable, and possible SUDEP deaths per 1,000 patient-years. Although this rate exceeds that expected in a healthy (nonepileptic) population matched for age and sex, it is within the range of estimates for epilepsy patients not receiving vagus nerve stimulation, ranging from 1.3 SUDEP deaths for the general population of patients with epilepsy, to 3.5 (for definite and probable) for a recently studied antiepileptic drug (AED) clinical trial population similar to the VNS Therapy System clinical cohort, to 9.3 for patients with medically intractable epilepsy who were epilepsy surgery candidates.

5. PRECAUTIONS — GENERAL

Physicians should inform patients about all potential risks and adverse events discussed in the VNS Therapy physician's manuals. Prescribing physicians should be experienced in the diagnosis and treatment of epilepsy and should be familiar with the programming and use of the VNS Therapy System. Physicians who implant the VNS Therapy System should be experienced performing surgery in the carotid sheath and should be trained in the surgical technique relating to implantation of the VNS Therapy System. The safety and effectiveness of the VNS Therapy System have not been established for use during pregnancy. VNS should be used during pregnancy only if clearly needed. The VNS Therapy System is indicated for use only in stimulating the left vagus nerve in the neck area inside the carotid sheath. The VNS Therapy System is indicated for use only in stimulating the **left vagus nerve below where the superior and inferior cervical cardiac branches separate from the vagus nerve**. It is important to follow infection control procedures. Infections related to any implanted device are difficult to treat and may require that the device be explanted. The patient should be given antibiotics preoperatively. The surgeon should ensure that all instruments are sterile prior to the procedure. Children 4-11 years of age may have a greater risk for infection when compared to adolescent and adult patients (≥ 12 years). Careful monitoring for site infection as well as the avoidance of manipulation of the surgical site post implant in children should be stressed. The VNS Therapy System may affect the operation of other implanted devices, such as cardiac pacemakers and implanted defibrillators. Possible effects include sensing problems and inappropriate device responses. If the patient requires concurrent implantable pacemaker, defibrillatory therapy or other types of stimulators, careful programming of each system may be necessary to optimize the patient's benefit from each device. Reversal of lead polarity has been associated with an increased chance of bradycardia in animal studies. It is important that the electrodes are attached to the left vagus nerve in the correct orientation. It is also important to make sure that leads with dual connector pins are correctly inserted (white marker band to + connection) into the generator's lead receptacles. The patient can use a neck brace for the first week to help ensure proper lead stabilization. Do not program the VNS Therapy System to an "ON" or periodic stimulation treatment for at least 14 days after the initial or replacement implantation. For Models 100, 101, 102 and 102R do not use frequencies of 5 Hz or below for long-term stimulation. Resetting the generator disables or turns the device OFF (output current = 0 mA). For Model 100, 101, 102 and 102R, resetting the generator will result in device history loss. Patients who smoke may have an increased risk of laryngeal irritation.

Generators with AutoStim only—Because the device senses changes in heart rate, false positive detection may cause unintended stimulation. Examples of instances where the heart rate may increase include exercise, physical activity, and normal autonomic changes in heart rate, both awake and asleep, etc. Adjustments to the AutoStim feature's detection threshold should be considered; which may include turning the feature OFF.

Generators with AutoStim only—The physical location of the device critically affects the feature's ability to properly sense heart beats. Care must be taken to follow the implant location selection process outlined in the Implantation Procedure.

Generators with AutoStim only—Talk to your patient about use of the AutoStim feature since use of the feature will result in faster battery drain and the potential for more frequent device replacements. The physician's manual describes the impacts to the battery life. The patient should return to their physician at appropriate intervals to further evaluate whether they are receiving benefit from the current AutoStim settings.

M1000 only — Since the Scheduled Programming feature allows the generator to apply therapy increases at scheduled intervals, it may not be appropriate for use in patients who are nonverbal or are unable to use the patient magnet to stop undesired stimulation. Similarly, exercise caution for use of this feature in patients with a history of obstructive sleep apnea, shortness of breath, coughing, swallowing difficulties, or aspiration.

6. ENVIRONMENTAL AND MEDICAL THERAPY HAZARDS

Patients should exercise reasonable caution in avoiding devices that generate a strong electric or magnetic field. If a generator ceases operation while in the presence of electromagnetic interference (EMI), moving away from the source may allow it to return to its normal mode of operation. VNS Therapy System operation should always be checked by performing device diagnostics after any of the procedures mentioned in the physician's manuals. For clear imaging, patients may need to be specially positioned for mammography procedures,

because of the location of the generator in the chest. Therapeutic radiation may damage the generator's circuitry, although no testing has been done to date and no definite information on radiation effects is available. Sources of such radiation include therapeutic radiation, cobalt machines, and linear accelerators. The radiation effect is cumulative, with the total dosage determining the extent of damage. The effects of exposure to such radiation can range from a temporary disturbance to permanent damage, and may not be detectable immediately. External defibrillation may damage the generator. Use of electrosurgery [electrocautery or radio frequency (RF) ablation devices] may damage the generator. Magnetic resonance imaging (MRI) should not be performed using a transmit RF body coil for certain VNS therapy device configurations or under certain specific conditions. In some cases, heating of the lead caused by the transmit RF body coil during MRI may result in serious injury. Static, gradient, and radio frequency (RF) electromagnetic fields associated with MRI may change the generator settings (i.e., reset parameters) or activate the VNS device if the Magnet Mode output remains "ON". Note that certain magnetic resonance (MR) system head coils operate in receive-only mode and require use of the transmit RF body coil. Other MR systems use a transmit/receive RF head coil. Local or surface coils may also be receive-only RF coils that require the transmit RF body coil for MRI. **The use of a receive RF coil does not alter hazards of the transmit RF body coil.** Exposure of the VNS Therapy System to any transmit RF coil must be avoided. Do not perform MRI scans using any transmit RF coil in the defined exclusion zones. See MRI with the VNS Therapy System instructions for use for details or further instructions for special cases such as lead breaks or partially explanted VNS Therapy systems. Extracorporeal shockwave lithotripsy may damage the generator. If therapeutic ultrasound therapy is required, avoid positioning the area of the body where the generator is implanted in the water bath or in any other position that would expose it to ultrasound therapy. If that positioning cannot be avoided, program the generator output to 0 mA for the treatment, and then after therapy, reprogram the generator to the original parameters. If the patient receives medical treatment for which electric current is passed through the body (such as from a TENS unit), either the generator should be set to 0 mA or function of the generator should be monitored during initial stages of treatment. Routine therapeutic ultrasound could damage the generator and may be inadvertently concentrated by the device, causing harm to the patient. For complete information related to home occupational environments, cellular phones, other environmental hazards, other devices, and ECG monitors, refer to the physician's manuals.

7. ADVERSE EVENTS — EPILEPSY

Adverse events reported during clinical studies as statistically significant are listed below in alphabetical order: ataxia (loss of the ability to coordinate muscular movement); dyspepsia (indigestion); dyspnea (difficulty breathing, shortness of breath); hypoesthesia (impaired sense of touch); increased coughing; infection; insomnia (inability to sleep); laryngismus (throat, larynx spasms); nausea; pain; paresthesia (prickling of the skin); pharyngitis (inflammation of the pharynx, throat); voice alteration (hoarseness); vomiting.

¹ The information contained in this Brief Summary for Physicians represents partial excerpts of important prescribing information taken from the physician's manuals. (Copies of VNS Therapy physician's and patient's manuals are posted at www.livanova.com.) The information is not intended to serve as a substitute for a complete and thorough understanding of the material presented in all of the physician's manuals for the VNS Therapy System and its component parts nor does this information represent full disclosure of all pertinent information concerning the use of this product, potential safety complications, or efficacy outcomes.

LivaNova USA, Inc.
100 Cyberonics Boulevard
Houston, Texas 77058
USA

Tel: +1 (281) 228-7200 / 1 (800) 332-137
Fax: +1 (281) 218-9332

www.livanova.com

© 2015-2021 LivaNova, PLC, London, UK.
All rights reserved.

LivaNova is a registered United States trademark of LivaNova, PLC. NCP, Demipulse™, Demipulse Duo™, Perennia™, VNS Therapy™, AspireHC™, PerenniaFLEX™, PerenniaDURA™, and AspireSR^v are registered trademarks of LivaNova USA, Inc. Pulse™, Pulse Duo™ and SenTiva™ are trademarks of LivaNova USA, Inc.

