



## SenTiva™

Information about your  
new VNS Therapy™ device

**VNS Therapy™ is a well established neuromodulation treatment for people with drug-resistant epilepsy.**



An add-on therapy for people with drug-resistant epilepsy



Implanted in a short surgical procedure lasting 1-2 hours<sup>2</sup>



Suitable for adults and children<sup>1</sup>



Safe and effective

## Introducing SenTiva™

All the benefits of previous generations of VNS Therapy™:

- ✓ Fewer seizures<sup>1</sup>
- ✓ Shorter seizures<sup>1</sup>
- ✓ AutoStim Mode
- ✓ Better recovery after seizures<sup>1</sup>
- ✓ Improved quality of life<sup>3</sup>
- ✓ SenTiva DUO™ available for patients with dual pin leads



### Scheduled Programming

Scheduled Programming allows your doctor to pre-program your VNS Therapy™ device to automatically increase therapy settings at intervals they choose. This option can reduce the need for attending follow up appointments for programming, giving you time back to live your life.



### Day-Night Programming

Your doctor can customise your VNS Therapy™ treatment based on your lifestyle preferences or side effect management by programming your device to different settings for any two periods of time during a 24-hour period.

## How does SenTiva™ work to control seizures?



### Normal Mode

Helps to reduce seizure frequency by delivering stimulation at regular intervals all day, every day




### AutoStim\* Mode

Helps to stop or shorten a seizure by responding to rapid heart rate increases, which may be associated with seizures



### Magnet Mode

Helps to stop or shorten a seizure once it starts by passing the VNS Therapy Magnet over the generator to deliver an on-demand stimulation

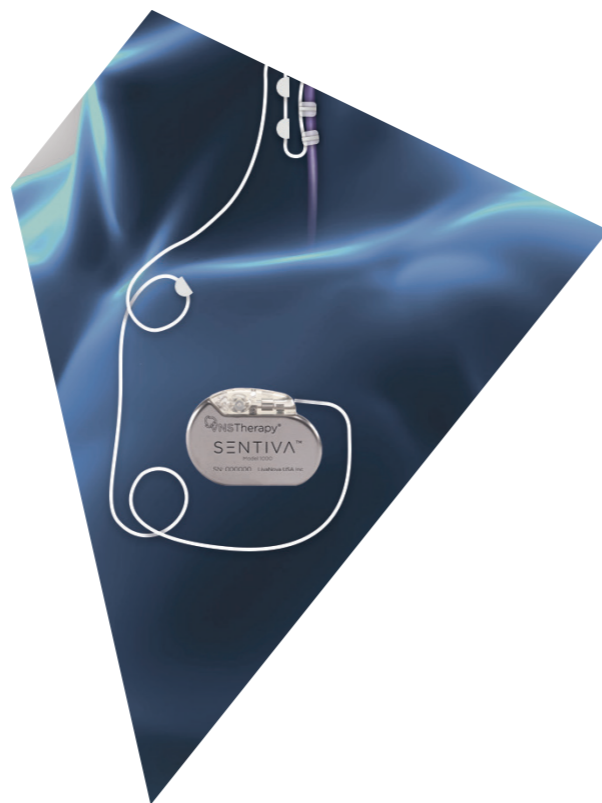

## Frequently Asked Questions - SenTiva™

1

### If I've had VNS Therapy™ before, will it feel different from my previous device?

Your doctor will programme the settings for AutoStim Mode in same way they are programming the settings for Normal Mode and Magnet Mode. If you think stimulation is coming on too much or too little, or if you feel discomfort, your doctor can adjust the settings appropriately.

2

### Will AutoStim Mode replace my magnet?

With SenTiva™ you can still use the magnet to receive extra stimulation or to stop your stimulation to manage side effects as with previous generators of VNS Therapy™.

3

### What happens when I exercise?

The detection system of SenTiva™ is designed to respond to rapid increases in heart rate. If you are exercising and your heart rate increases rapidly you may receive an extra dose of stimulation, but this will not harm you as it is very similar to receiving an extra stimulation via the Magnet Mode.

# Frequently Asked Questions - SenTiva™



4

## What if I don't tolerate the Scheduled Programming?

If you are unable to tolerate a scheduled therapy increase, your doctor should have instructed you that it is possible to temporarily stop stimulation by placing the magnet over the generator. Ensure that you contact your doctor or nurse immediately for programming adjustment.

5

## What if I don't tolerate the Day-Night Programming settings?

Your doctor or nurse will check that you can tolerate the setting before you leave the programming appointment.

## Brief Summary\* of Safety Information for Patients VNS Therapy™ System

[Epilepsy Indication] (August 2020)

### 1. INDICATIONS

The VNS Therapy System is indicated for use as an adjunctive therapy in reducing the frequency of seizures in patients whose epileptic disorder is dominated by partial seizures (with or without secondary generalization) or generalized seizures that are refractory to seizure medications. If you have the AspireSR® (Seizure Response) Model 106, SenTiva® Model 1000 or SenTiva DUO™ Model 1000-D device, it has a feature called the Automatic Stimulation Mode. This feature is for patients who experience seizures that are associated with an increase in heart rate. The feature can also be turned off by your physician, allowing the device to operate the same way as other VNS Therapy System models.

### 2. CONTRAINDICATIONS

**Vagotomy**— The VNS Therapy System should not be used (is contraindicated) in people who have had the left vagus nerve cut to treat another disorder (a left vagotomy).  
**Diathermy**— Inform anyone treating you that you CANNOT have any short-wave diathermy, microwave diathermy, or therapeutic ultrasound diathermy (hereafter referred to as "diathermy") anywhere on your body because you have an implanted VNS Therapy System (sometimes referred to as a "Vagus Nerve Stimulator" or "Vagus Nerve Stimulation"). Injury or damage can occur during diathermy treatment whether your VNS Therapy System is turned "ON" or "OFF." Diagnostic ultrasound is not included in this contraindication.

### 3. WARNINGS

**Avoid excessive vagus nerve stimulation** — Excessive stimulation of the vagus nerve can be produced by frequent magnet activation or more than 4 hours of continuous stimulation due to repeated magnet activations.

**Unapproved uses** — The safety and efficacy of the VNS Therapy System have not been established for uses outside its approved indications for use. The safety and efficacy of VNS Therapy have not been shown for people with these conditions: history of previous therapeutic brain surgery or brain injury, dysautonomias, lung diseases or disorders, including shortness of breath and asthma, ulcers (gastric, duodenal, or other), fainting (vasovagal syncope), irregular heartbeats (heart arrhythmias) or other heart abnormalities; other concurrent forms of brain stimulation; pre-existing hoarseness; progressive neurological diseases other than epilepsy or depression.

**Swallowing difficulties** — Difficulty swallowing may occur with active stimulation, and aspiration may result from the increased swallowing difficulties. Use of the magnet to temporarily stop stimulation while eating may mitigate the risk of aspiration.

**Shortness of breath** — Shortness of breath may occur with active VNS Therapy, especially if you have chronic obstructive pulmonary disease or asthma.

**Obstructive sleep apnea** — Use of the VNS Therapy device can cause or worsen pre-existing obstructive sleep apnea (episodes where breathing stops for short periods of time while sleeping). You should see your physician if you show any signs or symptoms of obstructive sleep apnea or worsening obstructive sleep apnea.

**Device malfunction** — Device malfunction could cause painful stimulation or direct current stimulation. Either event could cause nerve damage and other associated problems.

**Device removal** — Removal of the VNS Therapy System requires an additional surgical procedure. When a device is removed, the surgeon may leave part of the lead behind. This may pose certain risks.

**Device manipulation** — Do not manipulate the generator and lead through the skin, as this may damage or disconnect the lead from the generator and/or possibly cause damage to the vagus nerve.

**Device trauma** — Blunt trauma to the neck and/or any area of the body beneath which the lead is implanted could possibly cause damage to the lead.

**Not a cure** — The VNS Therapy System does not stop all seizures. Continue to avoid activities that can be hazardous to you and others, such as driving and swimming alone.

**Before having any MRI performed** — Call your doctor, so your VNS Therapy System can be discussed with the MRI personnel. In many cases, an MRI can be performed safely under certain conditions. However, for a few other cases, surgery may be required to remove the VNS Therapy System prior to an MRI. Before undergoing an MRI scan with your VNS Therapy System, the VNS system diagnostic information will be collected and the current turned off. The current will be turned on again after the scan is completed. Your doctor has access to detailed MRI-related information in the physician's manual.

**Patient Magnet is MR Unsafe** — Do not carry the patient magnet into the MR scanner room. The magnet could become a dangerous flying object if attracted by the strong magnetic field of the MRI scanner.

**Pain or other sensation during MRI scan** — If, during an MRI scan, you have any pain, discomfort, heating, or other unusual sensations, notify the MRI operator, so the MR procedure can be stopped.

**Cardiac Arrhythmia (Model 106 or 1000/1000-D only)** — If you have a cardiac arrhythmia, the Automatic Stimulation feature of the Model 106 is not suitable for you. This includes heart conditions or treatments that do not allow necessary changes in your heart rate, such as atrial fibrillation, pacemaker dependency, implantable defibrillator, or cardiac medications such as beta blockers.

### 4. PRECAUTIONS — IMPLANTABLE DEVICE: GENERAL

**Use during pregnancy** — The safety and effectiveness of the VNS Therapy System have not been established for use during pregnancy.

**Laryngeal irritation may result from stimulation** — Patients who smoke may have an increased risk of laryngeal (commonly called the "voice box") irritation.

**AutoStim Devices (Model 106 and 1000/1000-D)**

**Use during exercise** — Exercise or physical activity may trigger Automatic Stimulation if the feature is ON due to heart rate changes detected by the device.

**Heart Rate Changes Not Associated with Seizures** — Situations, including but not limited to exercise or physical activity, that cause rapid increases in heart rate may trigger Automatic Stimulation if the feature is ON.

If this is a concern, talk to your doctor about ways to stop stimulation during these situations. This could include using your magnet or having your doctor turn the AutoStim feature OFF.

**Battery Drain** — If your doctor has turned on the AutoStim feature, there will be a greater impact on battery life than if the feature is turned off, which may require more frequent generator replacements.

**AutoStim follow-up visits** — Use of the AutoStim feature will reduce battery life. Once the AutoStim feature has been activated, your doctor will work with you to determine a treatment plan to get to the most benefit.

**Time-based Features (Models 1000/1000-D only)** — Optional time-based features (e.g., Day-Night Programming, Scheduled Programming) do not automatically adjust for Day Light Savings Time or time zone changes. If you are using one of these features, you will need to go back to your doctor for reprogramming of the generator for any time changes.

### 5. PRECAUTIONS — IMPLANTABLE DEVICE: ENVIRONMENTAL & MEDICAL HAZARDS

Being close to certain types of equipment can affect the generator. Move away from or avoid equipment such as transmitting antennas.

**Pacemaker Warning signs** — Talk to your doctor before going into places with Pacemaker Warning signs.

**Small appliances** — Properly operating microwave ovens and other small electrical appliances, such as toasters, hair dryers, and electric shavers, should not affect the generator.

**Cellular phones** — Cellular phones can affect some implanted cardiac defibrillators and pacemakers, but tests to date show that they do not affect the generator.

**Transmitting devices** — Properly operating electrical ignition systems and power transmission lines should not affect the generator. Sources with high energy levels, such as transmitting antennas, may interfere with the device. Move at least 1.8 meters (6 feet) away from any equipment that interferes with your device.

**Antitheft devices, airport security systems, and other metal detectors** — Antitheft devices and metal detectors should not affect the generator or be affected by it. As a precaution, however, move through them at a steady pace; do not linger in the area and stay at least 40 centimeters (16 inches) away from such equipment.

**Electronic Article Surveillance (EAS) System tag deactivators** — The tag deactivators found in many retail stores can interfere with VNS Therapy when it is used near the generator. It can cause accidental activations or stop pulses. Stay at least 60 centimeters (2 feet) away from tag deactivators to avoid potential interference.

**Devices with strong electromagnetic fields** — Electrical or electromechanical devices with a strong static or pulsing magnetic field can cause the generator to start suddenly. Such devices may include strong magnets, tablet computers and their covers, hair clippers, vibrators, antitheft tag deactivators, and loudspeakers. Keep this type of equipment at least 20 centimeters (8 inches) away from your chest. If your generator stops while you are in a strong electromagnetic field, move away from the source so the device may return to regular operation.

Medical equipment, procedures, and surgery using certain electrical instruments can affect the VNS Therapy System's operation and sometimes damage the generator or lead.

Make sure that medical personnel know you have a device implanted in your chest. Always call your doctor before you have any medical tests that may affect, or be affected by, the VNS Therapy System as described in this section. Precautions may be needed.

**Routine diagnostic procedures** — Most routine diagnostic procedures, such as diagnostic ultrasound and radiography (x-rays), should not affect the VNS Therapy System.

**Mammography** — Because the generator is in your chest, you may need to be specially positioned for a mammogram. Otherwise, the device may be seen as a shadow on the mammogram. It could make a lesion or lump in that area hard or even impossible to detect. Make sure that your doctor and the mammography technician are aware of the implanted device.

**Radiation treatment** — Treatment with radiation, cobalt machines, and linear accelerators may damage the generator. No testing has been done to date. The effect of radiation on the device is not known. Talk with your doctor if you plan to have radiation treatment.

## EC Representative

### LIVANOVA BELGIUM NV

Ikaroslaan 83  
1930 Zaventem  
Belgium

Tel: +32.2.720.95.93

Fax: +32.2.720.60.53

[www.vnsththerapy.co.uk](http://www.vnsththerapy.co.uk)

## Manufacturer

### LIVANOVA USA, INC

100 Cyberonics Boulevard  
Houston, Texas 77058  
USA

Tel: +1.800.332.1375

Fax: +1.281.218.9332

[www.livanova.com](http://www.livanova.com)

Not approved in all geographies.

©2023 LivaNova USA, INC, a wholly-owned subsidiary of LivaNova PLC.  
All rights reserved. LivaNova® is a registered trademark of LivaNova USA, INC.  
VNS Therapy™ and SenTiva™ are trademarks of LivaNova USA, INC.  
EPI-2300373



0344

**Other procedures** — External cardiac defibrillation and other procedures for heart problems, as well as extracorporeal shockwave lithotripsy, diathermy, and electrocautery, may damage the generator. If you had any of these procedures and your doctor did not know about it, have the generator checked. While diagnostic ultrasound should not affect the VNS Therapy System, therapeutic ultrasound therapy could damage the generator or inadvertently harm you.

While the generator is stimulating or being set or tested, it may briefly interfere with nearby equipment. If this happens, move at least 1.8 meters (6 feet) away from such equipment.

**Radios and hearing aids** — The generator can interfere with devices that operate in the 30 kHz to 100 kHz range. Hearing aids and transistor radios operate in this range. In the theory, the generator could affect them, but no effects have yet been reported. No detailed testing has been done, so the effects are unknown.

**Other implanted devices** — The generator may affect other implanted medical devices, such as cardiac pacemakers and implantable defibrillators. Possible effects include sensing problems. These could lead to inappropriate responses from the generator.

## 6. PRECAUTIONS — MAGNETS

After your operation, your doctor will give you two magnets and accessories. The magnets contain a high-power magnet that is surrounded by a plastic casing in the shape of a watch. With normal use, they should remain powerful for approximately 3 years.

**Keep magnet with you** — Always carry the magnet with you. Show your family members or caregivers how to use it.

**Other implanted devices** — Do not place the magnet over a pacemaker since it may affect pacemaker function and could change the pacing rate. Do not place the magnet over a defibrillator (sometimes called ICD) since it could turn the device OFF.

**Damage from magnet** — Never put or store the magnets near credit cards, televisions, computers, computer disks, microwave ovens, watches, other magnets or items affected by strong magnetic fields. Keep them at least 25 centimeters (10 inches) away. If you are not sure how to use the magnet or have questions, ask your doctor to show you how.

## 7. SIDE EFFECTS

Adverse events reported during clinical studies as statistically significant are listed below in alphabetical order: ataxia (loss of the ability to coordinate muscular movement); dyspepsia (indigestion); dyspnea (difficulty breathing, shortness of breath); hypoesthesia (impaired sense of touch); increased coughing; infection; insomnia (inability to sleep); laryngismus (throat, larynx spasms); nausea; pain; paresthesia (prickling of the skin); pharyngitis (inflammation of the pharynx, throat); voice alteration (hoarseness); vomiting. Adverse events reported in clinical investigation of the AutoStim feature were comparable.

DHF1000-7031/1

## References:

1. VNS Therapy™ System Epilepsy Physician's Manual April 2021, LivaNova USA, Inc.
2. Patient's Guide for Epilepsy November 2021, LivaNova USA, Inc.
3. Orosz I., et al, 2014. Epilepsia, 55(10):1576-84.



LivaNova  
Epilepsy



VNS Therapy™